Alinity i

EBV VCA IgM Controls



Read Highlighted Changes: Revised March 2020.

NAME

Alinity i EBV VCA IgM Controls (also referred to as EBV VCA M Ctrls)

INTENDED USE

The Alinity i EBV VCA IgM Controls are for the estimation of test precision and the detection of systematic analytical deviations of the Alinity i analyzer when used for the qualitative detection of IgM antibodies to Epstein-Barr Virus (EBV) Viral Capsid Antigen (VCA) in human serum and plasma.

For additional information, refer to the Alinity i EBV VCA IgM reagent package insert and the Alinity ci-series Operations Manual.

CONTENTS

CONTROL - contains recalcified human plasma.

CONTROL + contains recalcified human plasma, reactive for anti-EBV VCA IgM.

Preservatives: ProClin 950 and sodium azide.

The controls are at the following ranges:

	EB <mark>V VCA Ig</mark> M	
Control	Quantity	S/CO
CONTROL -	1 x 8.0 mL	≤ 0.49
CONTROL +	1 x 8.0 mL	1.98 - 4.95

NOTE: The insert ranges for the controls are not lot specific and represent the total range of values which may be generated throughout the life of the product. It is recommended that each laboratory establish its own means and acceptable ranges which should fall within the package insert ranges. Sources of variation that can be expected include:

- Calibration
- Control lot
- Reagent lot

- Calibrator lot
- Instrument

PRECAUTIONS

- IVD
- For In Vitro Diagnostic Use

Safety Precautions

or potentially infectious components. Refer to the CONTENTS section of this package insert. No known test method can offer complete assurance that products derived from human sources or inactivated microorganisms will not transmit infection. Therefore, all human-sourced materials should be considered potentially infectious. It is recommended that this product and human specimens be handled in accordance with the OSHA Standard on Bloodborne Pathogens. Biosafety Level 2 or other appropriate biosafety practices should be used for materials that contain or are suspected of containing infectious agents. 1-4

 The human-sourced material used in the negative control is nonreactive for anti-EBV VCA IgM, HBsAg, anti-HIV-1/HIV-2, anti-HCV and HIV-1 RNA or HIV-1 Ag. The human-sourced material used in the positive control is reactive for anti-EBV VCA IgM and nonreactive for HBsAg, anti-HIV-1/HIV-2, anti-HCV and HIV-1 RNA or HIV-1 Ag.

The following warn	ings and precautions apply to: CONTROL - and
(
WARNING	Contains methylisothiazolone and sodium azide.
H317	May cause an allergic skin reaction.
EUH032	Contact with acids liberates very toxic gas
Prevention	
P261	Avoid breathing mist / vapors / spray.
P272	Contaminated work clothing should not be
	allowed out of the workplace.
P280	Wear protective gloves / protective
	clothing / eye protection.
Response	
P302+P352	IF ON SKIN: Wash with plenty of water.
P333+P313	If skin irritation or rash occurs: Get
	medical advice / attention.
P362+P364	Take off contaminated clothing and wash
	it before reuse.
Disposal	
P501	Dispose of contents / container in
	accordance with local regulations.

Safety Data Sheets are available at www.abbottdiagnostics.com or contact your local representative.

For a detailed discussion of safety precautions during system operation, refer to the Alinity ci-series Operations Manual, Section 8.

PREPARATION FOR USE

- This product is liquid ready-to-use.
- This product may be used immediately after removal from 2 to 8°C storage.
- · Prior to each use, mix by gentle inversion.

STORAGE

• Do not use past expiration date.

	Storage Temperature	Maximum Storage Time	Additional Storage Instructions
Unopened	2 to 8°C	Until expiration	
		date	
Opened	2 to 8°C	Until expiration	Store tightly capped.
		date	Return to refrigerated
			storage after use.



INSTRUMENT PROCEDURE

- To obtain the recommended volume requirements for the controls, hold the bottle vertically, and dispense 4 drops of the negative control and 4 drops of the positive control into each sample cup in the assigned position.
- For instructions on ordering and loading controls on the instrument, refer to the Alinity ci-series Operations Manual, Section 5.

INDICATIONS OF INSTABILITY OR DETERIORATION

Instability or deterioration should be suspected if there are precipitates, visible signs of leakage, turbidity, or if controls do not meet the appropriate package insert and/or Alinity ci-series Operations Manual criteria.


BIBLIOGRAPHY

- US Department of Labor, Occupational Safety and Health Administration, 29 CFR Part 1910.1030, Bloodborne pathogens.
- US Department of Health and Human Services. Biosafety in Microbiological and Biomedical Laboratories. 5th ed. Washington, DC: US Government Printing Office; December 2009.
- World Health Organization. Laboratory Biosafety Manual. 3rd ed. Geneva: World Health Organization; 2004.
- Clinical and Laboratory Standards Institute (CLSI). Protection of Laboratory Workers From Occupationally Acquired Infections; Approved Guideline—Fourth Edition. CLSI Document M29-A4. Wayne, PA: CLSI; 2014.

Note for number formatting:

- A space is used as thousands separator (example: 10 000 specimens).
- A period is used to separate the integer part from the fractional part of a number written in decimal form (example: 3.12%).

Key to Symbols

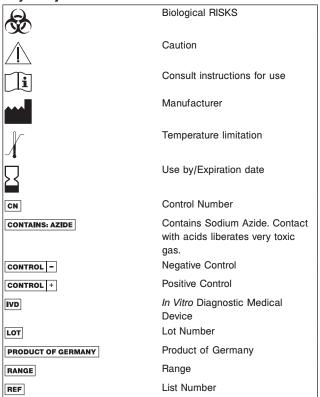

Alinity is a trademark of Abbott Laboratories in various jurisdictions. All other trademarks are property of their respective owners.





Customer Service: Contact your local representative or find country-specific contact information on www.abbottdiagnostics.com

Revised March 2020. ©2017, 2020 Abbott Laboratories

